


# Monoflex™

## INSTALLATION AND USER'S INSTRUCTIONS

ART NOS. SH120XS, SH120S, SH120M, SH120L, SH120XL,  
SH122XS, SH122S, SH122M, SH122L & SH122XL

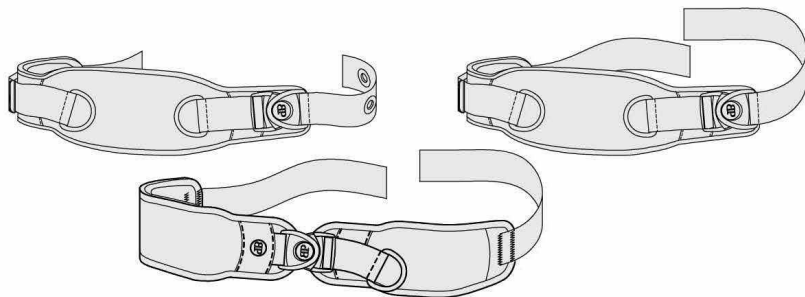

**These instructions provide important information for the safe use and maintenance of all Bodypoint Monoflex™ Chest Belts. Give these instructions to the user or their caregiver and review them to ensure that they are understood.**

**⚠ WARNING!** Product should be installed and fitted by a qualified rehab technician.

**⚠ WARNING!** Because of the risk of choking, it is dangerous to use this product without stabilizing the pelvis – always use with a properly fitted pelvic support belt.

### USE:

**⚠ WARNING!** This product should only be used for positioning a person in a wheelchair or work chair. It is NOT intended for use as a transportation safety device, as a personal restraint device, or in any other application where its failure could result in injury. Misuse of this product is unauthorized and unsafe.

**⚠ WARNING!** Accidental release of this chest belt can allow the user to slip down or fall from the wheelchair. If the user's movements or cognitive abilities could lead to accidental release, a caregiver must be present at all times during its use. Ensure that all caregivers know how to unfasten the product. Failure to do so may delay release in an emergency.

**⚠ WARNING!** As with any new seating support, this product may change the way a person sits. Users must continue to practice regular pressure relief activities and skin integrity checks, not only where this product


contacts the user, but also in primary pressure-bearing areas such as the sacrum, legs, and buttocks. If increased skin redness or irritation occurs, discontinue use and consult your physician or seating specialist. Failure to do so may result in serious injury, such as pressure ulcers.

**MAINTENANCE:** Check periodically for signs of wear in the stitching, webbing, and pads. If significant wear is found, contact your supplier for qualified repair or replacement by Bodypoint. Under no circumstance should this product be altered or repaired by unqualified persons – health and safety depend on it!



**CLEANING:** Machine wash, hot, 60°C (140°F). Do not bleach. Tumble dry, low temperature, or drip dry. Do not iron. (Placing the product inside a cloth bag during washing helps prevent scratches to the product and the machine.)


**WARRANTY:** This product carries a limited-lifetime warranty against defects in workmanship and materials arising under normal use by the original consumer. Contact your supplier or Bodypoint for warranty claims.

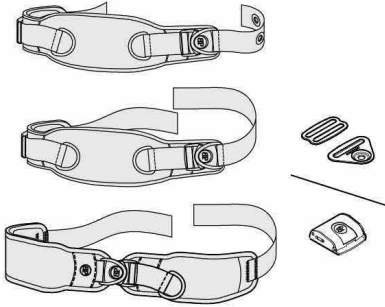

## PACKAGE CONTENTS

Monoflex™




Mounting straps with Cinch-mount™ or Flat-mount™, or Mounting straps with grommets



## POSITIONING




Seat user in wheelchair and establish correct posture with pelvic support belt. Determine desired position for the chest belt.

Position lower over the belly for more freedom of movement – position higher over the chest for more trunk control. When choosing position, consider interference with other devices.

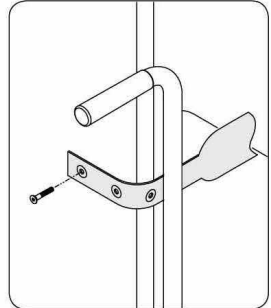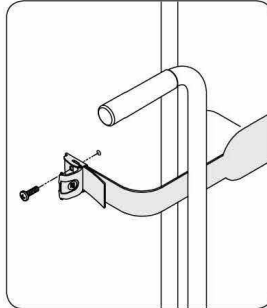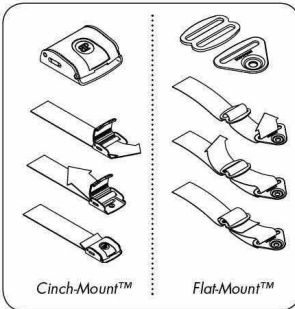

## DIRECT SCREW MOUNTING

Mounting straps can be attached directly to solid back surfaces. Use 6mm (1/4") Flat head or Button head screws to mount to chair frame or solid back. Mounting screws must have a minimum pullout strength of 90kg (200lbs). (Not included in package.)

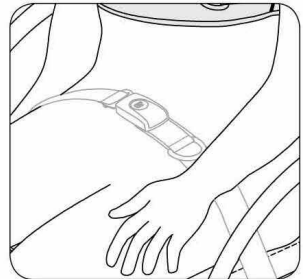

## BELT MOUNTING HARDWARE

Mounting straps can be attached using any type of Body-point belt mounting hardware with 6mm screws. (HW320 Band Clamps shown)

## ADJUSTMENT

With the user correctly seated, check the fit of the belt – it should be snug so the user is secure. Small adjustments in fit are done using the D-ring tightening straps. Large adjustments in fit are done using the mounting straps.

## SAFETY CHECK

When properly positioned in wheelchair, have user lean forward and side to side to check fit. Check for:

1. Normal operation of buckles and adjustment straps.
2. Comfort – If any rubbing occurs relocate straps.
3. Position – If too high or too low, adjust mounting location.
4. Interference with other devices – Relocate straps as necessary to clear armrests, accessory pads, or feeding tubes.